



OPEN

Platinum chloride-based viability RT-qPCR for SARS-CoV-2 detection in complex samples

Enric Cuevas-Ferrando^{1✉}, Walter Randazzo¹, Alba Pérez-Cataluña¹, Irene Falcó¹, David Navarro^{2,3}, Sandra Martin-Latil⁴, Azahara Díaz-Reolid¹, Inés Girón-Guzmán¹, Ana Allende⁵ & Gloria Sánchez¹

Isolation, contact tracing and restrictions on social movement are being globally implemented to prevent and control onward spread of SARS-CoV-2, even though the infection risk modelled on RNA detection by RT-qPCR remains biased as viral shedding and infectivity are not discerned. Thus, we aimed to develop a rapid viability RT-qPCR procedure to infer SARS-CoV-2 infectivity in clinical specimens and environmental samples. We screened monoazide dyes and platinum compounds as viability molecular markers on five SARS-CoV-2 RNA targets. A platinum chloride-based viability RT-qPCR was then optimized using genomic RNA, and inactivated SARS-CoV-2 particles inoculated in buffer, stool, and urine. Our results were finally validated in nasopharyngeal swabs from persons who tested positive for COVID-19 and in wastewater samples positive for SARS-CoV-2 RNA. We established a rapid viability RT-qPCR that selectively detects potentially infectious SARS-CoV-2 particles in complex matrices. In particular, the confirmed positivity of nasopharyngeal swabs following the viability procedure suggests their potential infectivity, while the complete prevention of amplification in wastewater indicated either non-infectious particles or free RNA. The viability RT-qPCR approach provides a more accurate ascertainment of the infectious viruses detection and it may complement analyses to foster risk-based investigations for the prevention and control of new or re-occurring outbreaks with a broad application spectrum.

The rapid spread of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) has led to an unprecedented global health and economic crisis. SARS-CoV-2 belongs to the *Coronaviridae* family, which includes enveloped RNA viruses causing respiratory, enteric, and systemic infections in a wide range of hosts, including humans and animals. Human coronaviruses have been traditionally considered responsible for endemic infections causing common cold symptoms, as in the cases of HKU1, 229E, OC43, and NL63 viruses, while more recently Middle East respiratory syndrome coronavirus (MERS-CoV) and SARS-CoV produced more severe epidemics in the Arabian Peninsula and in Asia. COVID-19 symptoms range from mild to severe, in which severe pneumonia and respiratory distress syndrome can lead to death. However, a significant number of infected people are asymptomatic, making the epidemiological control even more challenging.

SARS-CoV-2 is an airborne human pathogen primarily transmitted through droplets and aerosols, even though its detection in urine and faecal specimens raised the hypothesis of the possible fecal–oral transmission further sustained by the successful viral replication in cell culture^{1,2}. To control SARS-CoV-2 spread, extreme containment measures have been enforced worldwide along with several epidemiological surveillance strategies, which include tracing confirmed and suspected cases by clinical testing (e.g., SARS-CoV-2 nucleic acid or antigen tests on nasal or oral swabs or saliva samples), and monitoring community transmission by wastewater analysis (known as Wastewater Based Epidemiology, WBE)³.

In this context, several molecular assays based on real-time reverse transcriptase polymerase chain reaction (RT-qPCR) have been developed to detect and quantify SARS-CoV-2 RNA in clinical and environmental samples.

¹Department of Preservation and Food Safety Technologies, Institute of Agrochemistry and Food Technology, IATA-CSIC, Av. Agustín Escardino 7, 46980 Paterna, Valencia, Spain. ²Microbiology Service, Clinic University Hospital, INCLIVA Health Research Institute, Valencia, Spain. ³Department of Microbiology, School of Medicine, University of Valencia, Valencia, Spain. ⁴ANSES Laboratory for Food Safety, Université Paris-Est, 94700 Maisons-Alfort, France. ⁵Research Group on Quality and Safety of Fruits and Vegetables, Department of Food Science and Technology, CEBAS-CSIC, Campus Universitario de Espinardo, 25, 30100 Murcia, Spain. ✉email: enric.cuevas@iata.csic.es

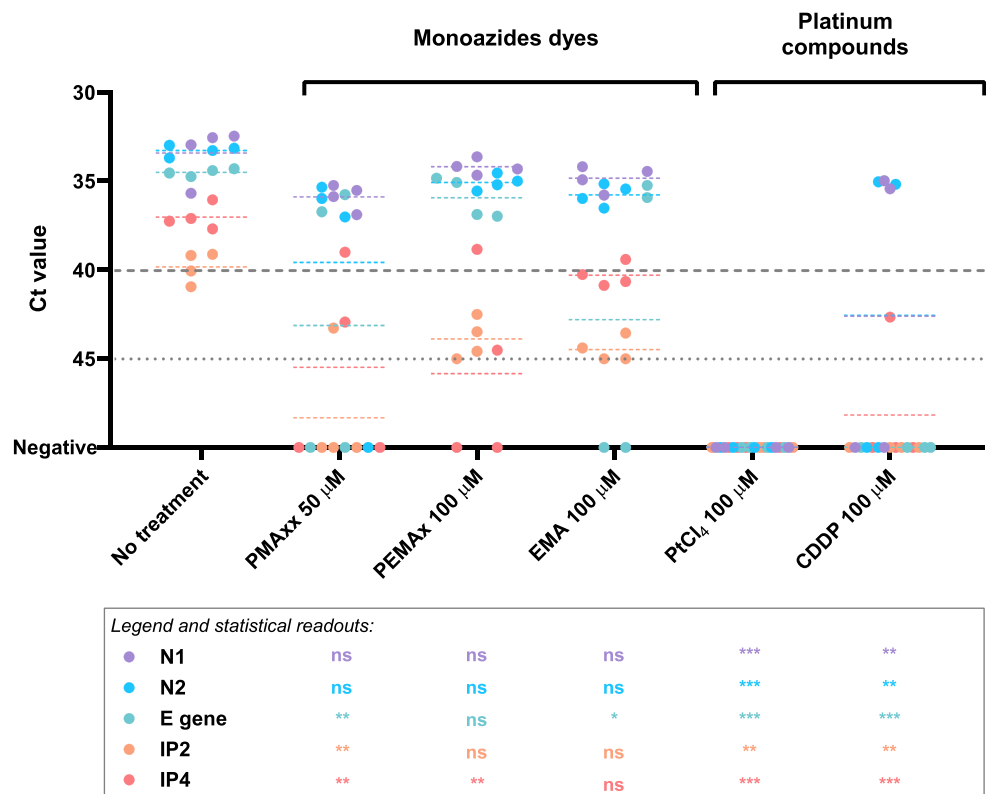


Figure 1. Performance of monoazide photoactivatable dyes and platinum compounds on SARS-CoV-2 genomic RNA assessed by targeting five different RNA regions. Dashed grey line represents RT-qPCR theoretical limit of detection for N1, N2 and gen E; dotted grey line represents RT-qPCR theoretical limit of detection for IP2 and IP4. Asterisks indicate significant difference from untreated control for each molecular target: * $p < 0.01$; ** $p < 0.001$; *** $p < 0.0001$; ns, not significant.

For instance, a test-based strategy (at least two consecutive negative RT-qPCR tests) has been widely adopted as a general public health guidance for release from (self-) isolation, reincorporation into the workplace, and patient transferral. However, COVID-19 patients can continue to shed viral RNA well beyond clinical recovery and persistent positive RT-qPCR does not necessarily indicate infectiousness⁴. In line, surveillance of SARS-CoV-2 by RT-qPCR in wastewaters is currently used as an effective tool to predict the prevalence of COVID-19 in communities. However, SARS-CoV-2 transmission through wastewater has not been demonstrated.

Besides being a rapid, easy-to-use, and cost-effective technique, RT-qPCR informs on the presence of viral RNA that does not correlate with infectivity, yet such testing is still being used as a surrogate marker of infectivity^{5–8}. On the contrary, viral replication in permissive cell line(s) is widely used to assess viral infectivity, and it has been readily available for SARS-CoV-2. Conversely, the facility requirements needed to handle SARS-CoV-2 infectious materials (biosafety level 3 laboratory, BSL-3), in addition to the low sensitivity and long turnaround time for results, typically from three to ten days, limited its extensive implementation for both clinical diagnosis and environmental risk assessment⁹.

Recently, novel molecular techniques, referred to as capsid integrity or viability qPCR assays incorporating viability markers such as monoazide dyes and metal compounds into qPCR-based methods, have been demonstrated to selectively remove false-positive qPCR signals deriving from free nucleic acids and virions with damaged capsids, finally allowing an estimation on viral infectivity¹⁰. However, the application of such techniques for enveloped viruses has not fully elucidated as it has failed for avian influenza virus (IAV) and infectious laryngotracheitis virus (ILTV) while it has recently been optimized for porcine epidemic diarrhea coronavirus^{11–13} and applied in environmental samples for SARS-CoV-2^{14–17}.

Results

Initial assessment of viability markers and RT-qPCR assays. With regard to the viability markers tested, platinum compounds were better at preventing PCR amplification of SARS-CoV-2 genomic RNA suspension than monoazide dyes, regardless of the RT-qPCR target (Fig. 1). Compared to untreated RNA, significant differences were detected for PtCl₄ and CDDP treated samples in all the five RT-qPCR targets tested. While PtCl₄ completely prevented the RNA amplification for all replicates, it occurred in 5 out of 20 CDDP treated replicates targeting N1, N2 and IP4. Among photoactivatable dyes, 50 μM PMAxx offered the best performance as it removed the signal in 8 replicates showing statistically significant differences for E gene, IP2 and IP4. An additional assay tested 100 μM PMAxx on SARS-CoV-2 genomic RNA without any improvement of the results

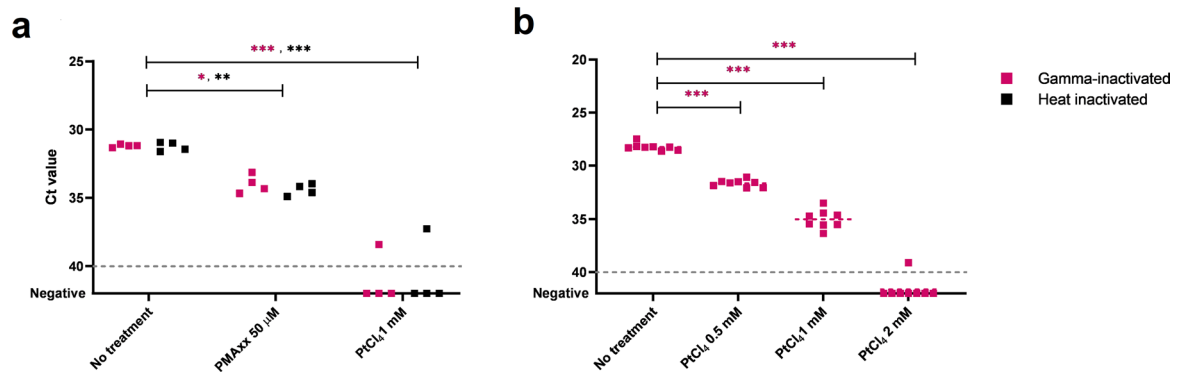


Figure 2. Assessment of viability markers on inactivated SARS-CoV-2 viral particles suspended in PBS buffer at different concentrations. RT-qPCR assays targeted N1 region. (a) Comparison of PMAxx and platinum chloride (PtCl₄) viability RT-qPCRs on low (ca. 10³ gc/mL) gamma- and heat inactivated SARS-CoV-2 viral particles. (b) Viability RT-qPCR optimization using increasing concentration of PtCl₄ on high concentrations of gamma-inactivated SARS-CoV-2 viral particles (ca. 10⁵ gc/mL). Dashed grey lines represent RT-qPCR theoretical limit of detection. Asterisks indicate significant difference from untreated control: **p* < 0.01; ***p* < 0.001; ****p* < 0.0001.

with respect to 50 μM PMAxx concentration (data not shown). EMA and PEMAxx completely removed RT-qPCR signals in 2 out of 20 replicates. Given these preliminary results, we further assessed PMAxx and PtCl₄ effect on SARS-CoV-2 gamma- (ca. 8.50 × 10⁵ gc/mL corresponding to 140 TCID₅₀/mL) and heat inactivated (ca. 1.88 × 10⁵ gc/mL corresponding to 80 TCID₅₀/mL) viral particles by using N1 as the most sensitive RT-qPCR assay among all the compared targets. PMAxx at 50 μM minimally reduced the PCR signals by 2.82 and 3.17 Cts with respect to the gamma- and heat inactivated controls, while the superior ability of PtCl₄ was confirmed for both gamma- and heat inactivated SARS-CoV-2 viral particles (Fig. 2). A final concentration of 1.0 mM PtCl₄ was needed to consistently prevent the amplification of inactivated viruses by viability RT-qPCR. Thus, we further applied the PtCl₄ viability RT-qPCR to high concentrated gamma-inactivated viral suspensions (ca. 8.50 × 10⁶ gc/mL). Results showed that 0.5 and 1.0 mM PtCl₄ reduced by 3.4 and 6.8 Cts compared to the control. Although significant statistical differences were detected for all treatments regardless of the concentration of the metal compound, only 2.0 mM PtCl₄ showed to consistently prevent signal amplification (only one positive out of 8 replicates, Ct = 39.11).

Effect of sample complexity on viability RT-qPCR. To determine the effect of sample matrix on viability RT-qPCR, we spiked tenfold diluted stool suspensions (1% w/v final dilution) and urine specimen (10% v/v final dilution) with approximately 10⁵ gc/mL gamma-inactivated SARS-CoV-2, and applied up to 5.0 mM PtCl₄ as viability marker. Compared to the untreated control, significant differences were observed for 1.0 mM PtCl₄ in urine samples or 1.25 mM PtCl₄ in stool suspensions (Fig. 3). However, a concentration of 5.0 mM was needed to completely remove the PCR signals in urine, while 2.5 mM PtCl₄ prevented the amplification of 1 out of 8 replicates in stool. Although the complete inhibition of amplification signals was achieved to a limited extent, a sharp difference above one logarithm of genomic copies (ΔCt ≈ 3.3) was observed in stool and urine samples processed with 1.25 and 3.75 mM PtCl₄, respectively.

Viability RT-qPCR validation on positive clinical samples and naturally contaminated wastewater. Additional experiments were set up to validate viability PtCl₄ RT-qPCR on nasopharyngeal swabs from COVID-19 positive patients and on naturally contaminated wastewater samples. Initial experiments using undiluted samples achieved unsuccessful results (data not showed), thus both clinical and wastewater samples were ten-fold diluted in PBS buffer. Nine tenfold diluted nasopharyngeal swabs and the corresponding heat-inactivated (95 °C for 10 min) subsamples were processed by RT-qPCR alone and viability RT-qPCR with either 1.0 or 2.5 mM PtCl₄ (Fig. 4). Applying 1.0 mM PtCl₄ viability RT-qPCR, consistent amplification signals were observed in both naïve and heat-treated samples with minimal Ct differences compared to RT-qPCR alone. Increased concentration to 2.5 mM led to a sharper discrimination of PCR signals (ΔCt = 9.24 ± 3.59). Similarly, the complete prevention of RT-qPCR signals occurred in one out of four samples at 1.0 mM PtCl₄, and in three out of five samples at 2.5 mM (Fig. 4). Regardless of the viability marker concentration applied, the complete prevention of amplification was observed in samples with initial low viral titer (Ct values ≥ 30). Moreover, the 2.5 mM PtCl₄ viability RT-qPCR was further validated on six wastewater samples naturally contaminated with SARS-CoV-2. The results showed that 2.5 mM PtCl₄ completely prevented the amplification in all samples (Fig. 5).

Discussion

Currently, research projects aiming to assess the risk of transmission and exposure to infectious virus either in clinical and environmental settings have been limited by the BSL-3 conditions needed to handle infectious SARS-CoV-2. The research effort of this investigation intended to provide a rapid and sensitive analytical method that selectively detects potentially infectious SARS-CoV-2 in a significantly shorter time than the traditional

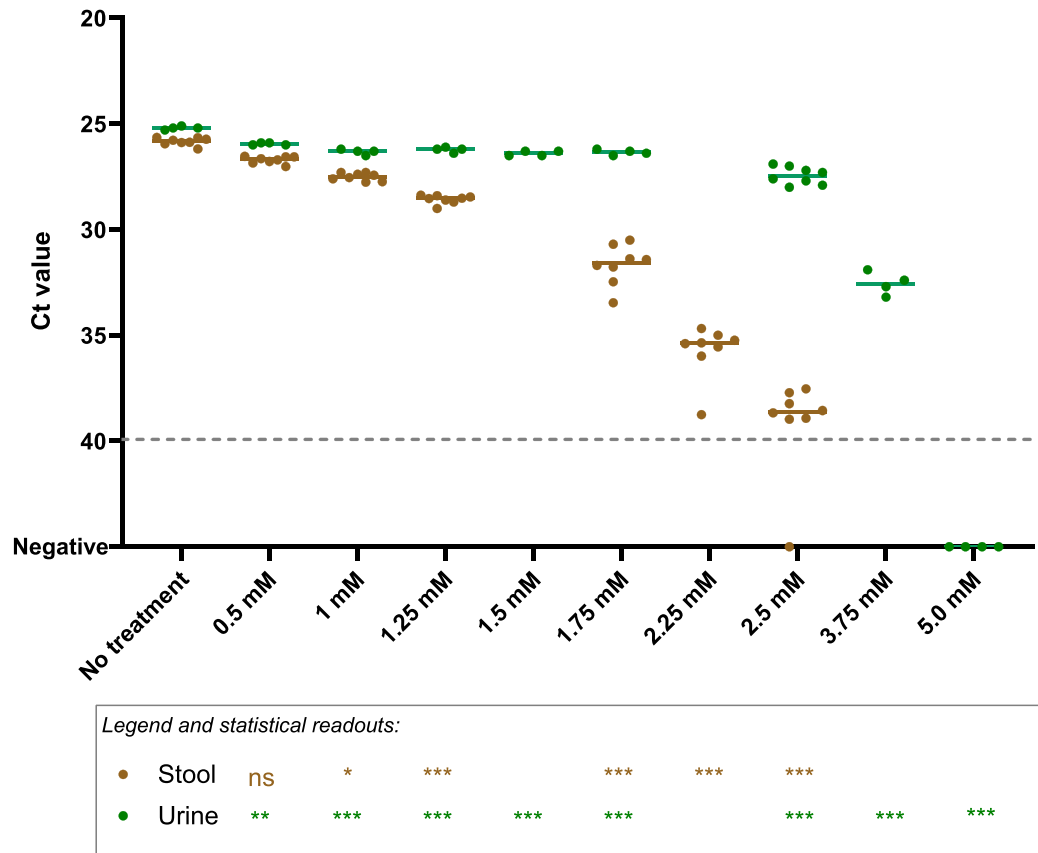


Figure 3. Platinum chloride (PtCl_4) viability RT-qPCR on ten-fold diluted faecal suspensions (1% w/v final dilution) (brown dots) and urine specimens (10% v/v final dilution) (green dots) spiked with approximately 10^5 gc/mL gamma-inactivated SARS-CoV-2. Dashed grey line represents RT-qPCR theoretical limit of detection. Asterisks indicate significant difference from untreated control: * $p < 0.01$; ** $p < 0.001$; *** $p < 0.0001$; ns, not significant.

cell-culture based method and that can be used in a wide range of applications, including clinical and environmental COVID-19 monitoring programs as epidemiological response to the pandemic that is causing such a public health emergency.

This study evaluated photoactivatable monoazide dyes and metal compounds as viability markers applied prior to nucleic acid extraction to prevent amplification of RNA from non-viable viral particles, thus enabling amplification only of viable/infectious viruses in downstream RT-qPCR assay. Selecting platinum chloride as the best performing viability marker, we demonstrated that viability RT-qPCR efficiently discriminated free RNAs and inactivated SARS-CoV-2 inoculated in buffer, stool and urine suspensions. Then, we further proved that the method inferred SARS-CoV-2 infectivity better than RT-qPCR alone in both nasopharyngeal swabs from positive COVID-19 patients and in naturally contaminated wastewater samples. In the case of complex matrices, increased PtCl_4 concentration of 2.5 mM and ten-fold sample dilution are recommended because of the high presence of organic matter, suspended solids, and inhibitors that hinder the efficacy of the viability treatment.

Our investigation initially included five well-established molecular assays since the length of the amplicon and/or the richness of secondary structures of targeted RNA may affect the efficiency of viability treatments^{18,19}. We show that metal compounds performed better than monoazide dyes, irrespective of RT-qPCR assays. However, RT-qPCR targeting N1 region is recommended because of its superior sensitiveness. This aspect is of importance because complex matrices needed to be diluted to achieve a more efficient inference of viral infectivity, as demonstrated in spiked stool and urine, in positive swabs and in contaminated wastewater. Similarly, sample dilution was needed to implement a viability RT-qPCR targeting norovirus in sewage²⁰. Moreover, N1 assay better fits the testing on samples with expected low viral concentrations (e.g., environmental samples) and/or PCR inhibitors (e.g., concentrated wastewater, stool). As N1 assay has been validated in many laboratories worldwide, this viability method could also be easily and widely implemented.

To the best of our knowledge, this is the first report comparing different conditions to optimize a rapid molecular assay independent from viral replication in cell culture developed to test SARS-CoV-2 infectivity in clinical and environmental samples. A recent investigation by our group demonstrated the suitability of viability RT-qPCRs to infer the infectivity of porcine epidemic diarrhea coronavirus, member of the genus *Alphacoronavirus* within *Coronaviridae* family¹³. Interestingly, we were able to demonstrate that PMAxx viability RT-qPCR

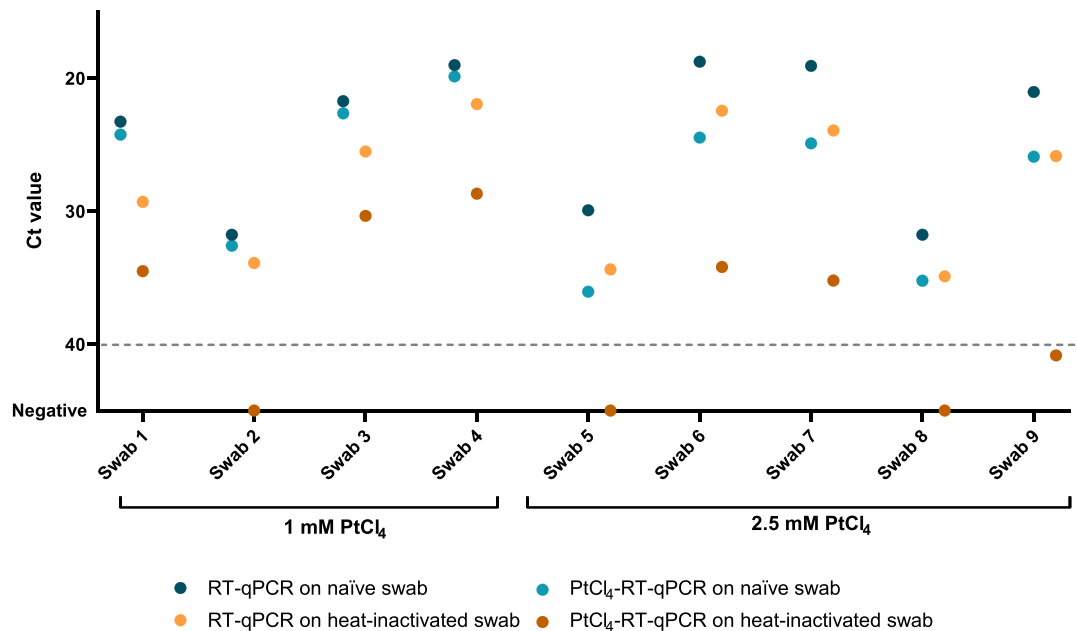


Figure 4. Validation of viability RT-qPCR with either 1 mM or 2.5 mM PtCl₄ on ten-fold diluted nasopharyngeal swabs from COVID-19 positive patients. Plotted dots represents the median cycle threshold value (Ct) of naïve and heat-inactivated (95 °C for 10 min) subsamples assayed by RT-qPCR alone and viability RT-qPCR both targeting N1. Dashed grey line represents RT-qPCR theoretical limit of detection.

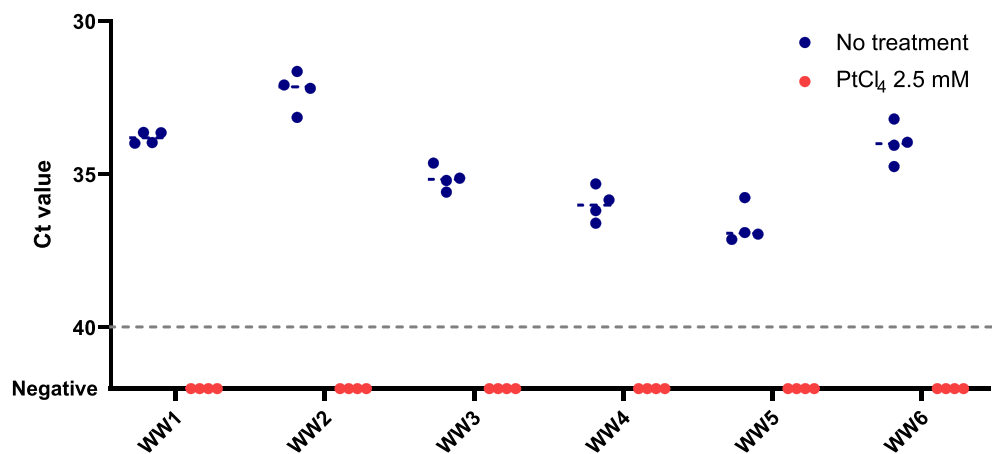


Figure 5. Validation of 2.5 mM PtCl₄ viability RT-qPCR on ten-fold diluted naturally contaminated wastewater samples. Dashed grey line represents RT-qPCR theoretical limit of detection.

matched the thermal inactivation pattern obtained by cell culture better than other viability markers, including PtCl₄ and RT-qPCR alone. Vu Duc Cahn et al. 2021 identified CDDP at a concentration of 100 µM as the most efficient reagent for the selective detection of infectious murine hepatitis virus (MHV, used as SARS-CoV-2 surrogate) by RT-qPCR²¹. Alternative rapid methods to assess the viability of enveloped viruses have been explored with inconclusive results. These included propidium monoazide and immunomagnetic separation tested on laryngotracheitis virus and ethidium monoazide on avian influenza virus^{11,12}. It is worth to report that during the reviewing process of this study few studies have been reporting the use of PMA or PMAxx to discriminate live and dead SARS-CoV-2 in environmental samples^{15–17}.

Our viability RT-qPCR results of nasopharyngeal swabs from positive COVID-19 patients indicate the potential infectivity of the samples, while naturally contaminated wastewater are unlikely to contain infectious viral particles. These later findings reflect the viral replication in cell culture from RNA positive stool and respiratory samples as well as the unsuccessful attempts to isolate and cultivate SARS-CoV-2 from wastewater samples^{22–24}.

Our findings are clinically relevant as RT-qPCR has become the primary method to diagnose COVID-19. However, as it detects RNA, its ability to determine the infectivity of patients is limited^{5–8}. In addition, the immune system can neutralise SARS-CoV-2 preventing subsequent infection but not eliminating nucleic acid,

which degrades slowly over time. This has been confirmed in cohort studies that concluded that seroconversion does not necessarily lead to the elimination of viral RNA, with cases being RT-PCR positive up to > 63 days after symptom onset despite having neutralizing antibodies^{25–27}. Furthermore, some reports correlated the infectiousness of upper respiratory tract samples with RT-qPCR Ct values in COVID-19 cases. Analysing a large dataset (n = 324), Singanayagam and colleagues demonstrated that the probability of viral recovery from samples with $27.5 < Ct < 30$ was $\approx 66\%$, decreasing to $\approx 28\%$ for $30 < Ct < 35$, and to 8.3% for $Ct > 35$ ²⁴. Similarly, Bullard observed SARS-CoV-2 cell infectivity only for respiratory specimens sampled < 8 days symptom onset with $Ct < 24$ ²⁸. However, viral replication was also obtained from samples with elevated Ct values of 36–39^{7,29}. Notwithstanding, the correlation between RNA and virus isolation remains unclear.

Unfortunately, we had no access to clinical samples with higher Ct values which are likely to contain non-infectious particles to contrast such hypothesis by the proposed viability RT-qPCR. In addition, the ratio between viral shedding and infectivity has been reported to vary along the course of the infection^{4,6,23}. This information regarding epidemiological characteristics, symptom history and relevant sampling details included in medical records could have explained at least in part the different performances of viability RT-qPCR among clinical samples, however it could not be retrieved as de-identified specimens were analysed in this study.

Despite the viability treatment, we detected residual signals in heat inactivated nasopharyngeal swabs. This could be attributed to the viral envelop and nucleoproteins that limit the access and/or the binding of viability markers to SARS-CoV-2 RNA, as hypothesised for avian influenza virus and bacteriophage T4^{12,30}. The enveloped structure of coronaviruses may also explain the increased concentration of viability markers needed for SARS-CoV-2 and PEDV compared to human enteric viruses^{13,20}. This cumbersome finding obtained by the proposed viability procedure suggests that the overestimation of the infectivity of a given sample may occur which, although warranting a careful interpretation, represents a conservative prediction. Despite the fact that this pretreatment is a step forward to better interpret quantification of SARS-CoV-2, improvements in the procedure needs to be undertaken. For instance, it has recently suggested to combine viability dyes with surfactants^{13,31}. Moreover, by collecting clinical samples in PBS buffer has the disadvantage in terms of biohazard samples management.

With regards to wastewater samples that tested positive for SARS-CoV-2 RNA, they most probably contained detergents and chemicals that are detrimental to viral infectivity further supporting the efficacy of the viability RT-qPCR in discriminating potentially infectious and inactivated viral particles³². The ultimate confirmation on the infectivity of the samples by cell culture, although recommendable, could not be provided. Nonetheless, recent laboratory scale investigations on SARS-CoV-2 persistence in wastewater estimated that the infectious titer of spiked virus decreases by one logarithm (T90) in 1.5–1.9 days at room temperature, and in few minutes at higher temperatures^{33,34}. This evidence suggests that naturally contaminated wastewater samples are unlikely to contain infectious particles. Detection of SARS-CoV-2 by either culture and viability RT-qPCR is valuable as a proxy for infectiousness; however, as the human infectious dose remains unknown, the significance of low titres of infectious virus for human-to-human transmission remains uncertain. Above all, as some individuals reportedly remain PCR positive weeks after SARS-CoV-2 infection recovery, knowing whether viral RNA in these persistent carriers is contagious provides key insights for quarantine policy, to safely discontinue self-isolation and contact tracing as essential public health measures to definitively prevent transmission^{6,27,35}. Besides some limitations, the proposed viability RT-qPCR effectively reduced the amplification signals of non-infectious and free RNA of SARS-CoV-2 in complex matrices finally providing a better estimation of the infectiousness of samples. Thus, mathematical models derived from laboratory scale experiments comparing viability RT-qPCR and viral replication could correlate viral load and infectivity, finally providing relevant tools of interest based on rapid molecular assay for prevention strategies and risk assessment.

In conclusion, the use of pre-treatments to prevent RT-qPCR amplification of RNA from non-infectious SARS-CoV-2 using platinum chloride as a viability marker of infectivity was implemented in stool and urine samples and successfully validated in naturally contaminated wastewater samples, supporting the idea that SARS-CoV-2 present in sewage is not infectious. Residual amplification signals in nasopharyngeal swabs exposed to heat-inactivation overestimated the amount of viable virus, still providing a conservative interpretation of the infectiousness of the sample. The authors believe that the described platinum-based viability RT-qPCR method would be of great use in the research field, especially when involving environmental samples such as wastewater. As a limitation, the high viral loads that characterize nasopharyngeal samples from infected individuals resulted in less reliable outcomes thus making the method not optimal for clinical monitoring routines. Even so, as for future work, it would be interesting to apply this protocol in samples from infected patients who have already been vaccinated or are in the final stage of the disease and therefore present higher Cq values.

Overall, our study proposes a rapid analytical tool based on viability RT-qPCR to infer SARS-CoV-2 infectivity with potential application in risk assessment, and prevention and control in public health programmes.

Methods

Viral materials, viability markers and optimization of viability treatment. SARS-CoV-2 genomic RNA (VR-1986D™, ATCC, VA, US), gamma-irradiated (5×10^6 RADs)

(NRC-52287, BEI Resources, VA, US) and heat inactivated (65 °C for 30 min) (NR-52286, BEI Resources, VA, US) viral particles preparations all obtained from isolate USA-WA1/2020 were used for initial screening of viability markers. Specifically, monoazide photoactivatable dyes and platinum compounds were initially screened as viability marker candidates using SARS-CoV-2 genomic RNA, gamma-inactivated, and heat inactivated SARS-CoV-2 suspensions. Viability marker stock solutions were prepared as follows and stored at -20 °C for later use: ethidium monoazide (EMA™, Geniul, Spain) was diluted in dimethylsulfoxide (DMSO) to 2.0 mM, PEMAX™ (Geniul, Spain) and propidium monoazide (PMAxx™, Biotium, CA, US) were diluted in nuclease-free water to 4.0 mM, platinum (IV) chloride (PtCl₄; Acros Organics, NJ, US) and cis-diamineplatinum (II) dichloride (CDDP;

Sigma-Aldrich, MO, US) salts were dissolved in DMSO to 1.0 M and further diluted in nuclease-free water to 50 mM. Viability assays were carried out by treating 300 μ L of either genomic SARS-CoV-2 RNA (approx. 10^3 gc/mL), gamma-inactivated (approx. 10^5 gc/mL), and heat inactivated SARS-CoV-2 (approx. 10^5 gc/mL) suspensions with final concentrations of 50–100 μ M photoactivatable dyes (PMAxx™, PEMAX™, or EMA™) or 0.1–2.0 mM platinum compounds (CDDP or PtCl₄) in DNA LoBind tubes (Eppendorf, Germany). Photoactivation of mono-azide dyes was achieved by 10 min of dark-incubation in an orbital shaker (150 rpm) at room temperature (RT) followed by 15 min blue LED light exposure in a photo-activation system (Led-Active Blue, GenIUL). Alternatively, 30 min incubation at RT in an orbital shaker (150 rpm) were used for viability treatments with platinum compounds. A control consisting of genomic RNA or virus suspension without viability marker was included in each assay. Following the viability treatment, the viral RNA was immediately purified as described hereafter.

Assessment of PtCl₄ viability RT-qPCR in artificially inoculated and validation in naturally contaminated samples. Platinum (IV) chloride was selected as the most reliable viability marker and tested at final concentrations of 0.5 to 5.0 mM for viability RT-qPCR optimization in stool, urine, nasopharyngeal swabs and wastewater samples.

For the initial optimization, stool and urine specimens that had tested negative for SARS-CoV-2 were retrieved from IATA biobank. Faecal material was resuspended 1% w/v in phosphate-buffered saline (PBS), and supernatant recovered by centrifugation at 2000 \times g for 5 min. Direct and ten-fold diluted urine, and ten-fold diluted faecal suspension (final 1% w/v faecal dilution) were spiked with either gamma- and/or heat inactivated SARS-CoV-2 to approximately 10^5 gc/L final concentration.

Then, nasopharyngeal swabs from positive COVID-19 patients and naturally contaminated wastewater samples were used to validate the viability PtCl₄ RT-qPCR. Nasopharyngeal swabs (n = 9) from COVID-19 positive patients were originally collected at Hospital Clínico Universitario de Valencia (Valencia, Spain) and included in this study once de-identified. To test whether the detection of viral RNA was exclusive for infectious particles, nasopharyngeal swab subsamples were inactivated at 95 °C for 10 min, included in the experiments along with naïve specimen and both assayed by RT-qPCR and viability PtCl₄ RT-qPCR.

SARS-CoV-2 positive wastewater grabbed samples (n = 6) were collected in June–October, 2020 from different wastewater treatments plants involved in a WBE monitoring programme. The samples were originally concentrated by an aluminium precipitation procedure and tested positive for at least two RT-qPCR targets (N1, IP4 or E gene)³⁶. To exclude additional viral inactivation due to the concentration procedure, wastewater were freshly concentrated by Centricon-Plus 70 centrifugal ultrafilters units with a cut-off of 100 kDa (Merk-Millipore, MA, US)³⁷. Samples were all diluted in PBS as specified. Viability treatment, RNA extraction and SARS-CoV-2 detection were carried out as hereafter detailed.

Viral RNA purification and SARS-CoV-2 detection. Viral RNA was extracted using Maxwell® RSC 16 instrument and Maxwell RSC Pure Food GMO and authentication kit (Promega, Spain) and detected by RT-qPCR targeting N1, N2, E gene, IP2 and IP4 regions³⁸. Viral RNA from nasopharyngeal samples was extracted using a KingFisher™ Flex (Thermo Fisher Scientific) instead. Given the superior sensitivity of N1 RT-qPCR resulting from the initial screening, this target was used for subsequent determinations. Each RT-qPCR assay was performed in duplicate and included nuclease-free water as negative control, and SARS-CoV-2 complete genomic RNA (VR-1986D™, ATCC, VA, US), E gene plasmid (10006896, 2019-nCoV_E Positive Control from Charité/Berlin, IDT, Belgium) or N1/N2 plasmid (10006625, 2019-nCoV_N_Positive Control from CDC, IDT, Belgium) as positive controls. Ten-fold RNA dilutions were consistently tested to check RT-qPCR inhibition due to viability marker residues or inhibitory substances in the sample.

Statistical analysis. All data were compiled from three independent experiments with at least two technical replicates for each variable. Data are presented as median \pm SD. Significant differences in median cycle threshold (Ct) were determined by using either one- or two way(s) ANOVA followed by Dunnett's multiple comparisons test on GraphPad Prism version 8.02 (GraphPad Software, US). Differences in means were considered significant when the *p* was < 0.05.

Ethics statement. The current study was approved by the Research Ethics Committee of Hospital Clínico Universitario INCLIVA (March, 2020).

Received: 21 June 2021; Accepted: 24 August 2021

Published online: 13 September 2021

References

- Meselson, M. Droplets and aerosols in the transmission of SARS-CoV-2. *N. Engl. J. Med.* **382**, 2063 (2020).
- Guo, M., Tao, W., Flavell, R.A. *et al.* Potential intestinal infection and faecal–oral transmission of SARS-CoV-2. *Nat Rev Gastroenterol Hepatol.* **18**, 269–283 (2021).
- Bivins, A. *et al.* Wastewater-based epidemiology: Global collaborative to maximize contributions in the fight against COVID-19. *Environ. Sci. Technol.* **54**(13), 7754–7757 (2020).
- Owusu, D. *et al.* Persistent SARS-CoV-2 RNA shedding without evidence of infectiousness: A cohort study of individuals with COVID-19. *J. Infect. Dis.* **jiab107** (2021).
- Atkinson, B. & Petersen, E. SARS-CoV-2 shedding and infectivity. *Lancet* **395**, 1339–1340 (2020).
- Widders, A., Broom, A. & Broom, J. SARS-CoV-2: The viral shedding vs infectivity dilemma. *Infect. Dis. Heal.* **25**, 210–215 (2020).
- Romero-Gómez, M. P. *et al.* Ct value is not enough to discriminate patients harbouring infective virus. *J. Infect.* **82**(3), e35–e37 (2021).

8. Krupp, K., Madhivanan, P. & Perez-Velez, C. M. Should qualitative RT-PCR be used to determine release from isolation of COVID-19 patients?. *J. Infect.* **81**, 452–482 (2020).
9. Ogando, N. S. *et al.* SARS-coronavirus-2 replication in Vero E6 cells: Replication kinetics, rapid adaptation and cytopathology. *J. Gen. Virol.* **101**(9), 925–940 (2020).
10. Leifels, M. *et al.* Capsid integrity quantitative PCR to determine virus infectivity in environmental and food applications—A systematic review. *Water Res.* **X** **222**, 182 (2020).
11. Bindari, Y. R., Walkden-Brown, S. W. & Gerber, P. F. Methods to prevent PCR amplification of DNA from non-viable virus were not successful for infectious laryngotracheitis virus. *PLoS ONE* **15**(5), e0232571 (2020).
12. Graiver, D. A., Saunders, S. E., Topliff, C. L., Kelling, C. L. & Bartelt-Hunt, S. L. Ethidium monoazide does not inhibit RT-PCR amplification of nonviable avian influenza RNA. *J. Virol. Methods.* **164**(1–2), 51–4 (2010).
13. Puente, H., Randazzo, W., Falcó, I., Carvajal, A. & Sánchez, G. Rapid selective detection of potentially infectious porcine epidemic diarrhea coronavirus exposed to heat treatments using viability RT-qPCR. *Front. Microbiol.* **11**, 1911 (2020).
14. Cuevas-Ferrando, E. *et al.* Discrimination of non-infectious SARS-CoV-2 particles from fomites by viability RT-qPCR. *Environ. Res.* **203**, 111831 (2021).
15. Polo, D., Lois, M., Fernández-Núñez, M. T. & Romalde, J. L. Detection of SARS-CoV-2 RNA in bivalve mollusks and marine sediments. *Sci. Total Environ.* **786**, 147534 (2021).
16. Hong, W. *et al.* Rapid determination of infectious SARS-CoV-2 in PCR-positive samples by SDS-PMA assisted RT-qPCR. *Sci. Total Environ.* **797**, 149085 (2021).
17. Wurtzer, S. *et al.* Several forms of SARS-CoV-2 RNA can be detected in wastewaters: Implication for wastewater-based epidemiology and risk assessment. *Water Res.* **198**, 117183 (2021).
18. Contreras, P. J., Urrutia, H., Sossa, K. & Nocker, A. Effect of PCR amplicon length on suppressing signals from membrane-compromised cells by propidium monoazide treatment. *J. Microbiol. Methods* **87**, 89–95 (2011).
19. Soejima, T., Schlitt-Dittrich, F. & Yoshida, S.-I. Polymerase chain reaction amplification length-dependent ethidium monoazide suppression power for heat-killed cells of Enterobacteriaceae. *Anal. Biochem.* **418**, 37–43 (2011).
20. Randazzo, W., López-Gálvez, F., Allende, A., Aznar, R. & Sánchez, G. Evaluation of viability PCR performance for assessing norovirus infectivity in fresh-cut vegetables and irrigation water. *Int. J. Food Microbiol.* **229**, 1–6 (2016).
21. Canh, V. D., Torii, S., Yasui, M., Kyuwa, S. & Katayama, H. Capsid integrity RT-qPCR for the selective detection of intact SARS-CoV-2 in wastewater. *Sci. Total Environ.* **791**, 148342 (2021).
22. Rimoldi, S. G. *et al.* Presence and infectivity of SARS-CoV-2 virus in wastewaters and rivers. *Sci. Total Environ.* **744**, 140911 (2020).
23. Wölfel, R. *et al.* Virological assessment of hospitalized patients with COVID-2019. *Nature* **581**, 465–469 (2020).
24. Singanayagam, A. *et al.* Duration of infectiousness and correlation with RT-PCR cycle threshold values in cases of COVID-19, England, January to May 2020. *Eur. Commun. Dis. Bull.* **25**(32), 2001483 (2020).
25. Molina, L. P., Chow, S.-K., Nickel, A. & Love, J. E. Prolonged detection of severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) RNA in an obstetric patient with antibody seroconversion. *Obstet. Gynecol.* **136**, 838–841 (2020).
26. Liu, W.-D. *et al.* Prolonged virus shedding even after seroconversion in a patient with COVID-19. *J. Infect.* **81**, 318–356 (2020).
27. Vibholm, L. K. *et al.* SARS-CoV-2 persistence is associated with antigen-specific CD8 T-cell responses. *EBioMedicine* **64**, 103230 (2021).
28. Bullard, J. *et al.* Predicting infectious SARS-CoV-2 from diagnostic samples. *Clin. Infect. Dis. Off. Publ. Infect. Dis. Soc. Am.* **71**(10), 2663–2666 (2020).
29. Clinical and virologic characteristics of the first 12 patients with coronavirus disease 2019 (COVID-19) in the United States. *Nat. Med.* **26**, 861–868 (2020).
30. Fittipaldi, M. *et al.* Discrimination of infectious bacteriophage T4 virus by propidium monoazide real-time PCR. *J. Virol. Methods.* **168**(1–2), 228–232 (2010).
31. Hong W. *et al.* Rapid determination of infectious SARS-CoV-2 in PCR-positive samples by SDS-PMA assisted RT-qPCR. *Sci. Total Environ.* **797**, 149085 (2021).
32. Khokhar, M., Roy, D., Purohit, P., Goyal, M. & Setia, P. Viricidal treatments for prevention of coronavirus infection. *Pathog. Glob. Health* **114**, 349–359 (2020).
33. Bivins, A. *et al.* Persistence of SARS-CoV-2 in water and wastewater. *Environ. Sci. Technol. Lett.* **7**, 937–942 (2020).
34. de Oliveira, L. C. *et al.* Viability of SARS-CoV-2 in river water and wastewater at different temperatures and solids content. *Water Res.* **195**, 117002 (2021).
35. Esteve, C., Catherine, F. X., Chavanet, P., Blot, M. & Piroth, L. How should a positive PCR test result for COVID-19 in an asymptomatic individual be interpreted and managed?. *Médecine Mal. Infect.* **50**, 633–638 (2020).
36. Randazzo, W. *et al.* SARS-CoV-2 RNA in wastewater anticipated COVID-19 occurrence in a low prevalence area. *Water Res.* **181** (2020).
37. Medema, G., Heijnen, L., Elsinga, G., Italiaander, R. & Brouwer, A. Presence of SARS-coronavirus-2 RNA in sewage and correlation with reported COVID-19 prevalence in the early stage of the epidemic in the Netherlands. *Environ. Sci. Technol. Lett.* **7**, 511–516 (2020).
38. Pérez-Cataluña, A. *et al.* Comparing analytical methods to detect SARS-CoV-2 in wastewater. *Sci. Total Environ.* **758**, 143870 (2021).

Acknowledgements

The study was supported by CSIC (202070E101), Generalitat Valenciana (Covid_19-SCI), MICINN co-founded by AEI/FEDER, UE (AGL2017-82909), and MICINN/AEI (PID2019-105509RJ-I00). EC-F is recipient of a pre-doctoral contract from the MICINN, Call 2018. We thank Agustin Garrido Fernández and Andrea Lopez de Mota at IATA-CSIC for providing support in sample processing. We acknowledge Global Omnium S.L., NILSA, Aguas de Malaga, ESAMUR and FACSA for coordinating and managing wastewater sampling.

Author contributions

G.S., A.A. and W.R. conceived the study with input from D.N., A.P.-C., I.F., S.M.L. and E.C.-F. E.C.-F., I.F., A.D.-R., and I.G.-G. led data acquisition. D.N. provided the nasopharyngeal swabs from COVID-19 positive patients. G.S., E.C.-F., and W.R. led data analysis, interpretation, and visualisation. E.C.-F. and W.R. wrote the draft report, and all other authors revised the report critically for important intellectual content. All authors critically reviewed and approved the final version of the manuscript.

Competing interests

The authors declare no competing interests.

Additional information

Correspondence and requests for materials should be addressed to E.C.-F.

Reprints and permissions information is available at www.nature.com/reprints.

Publisher's note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

© The Author(s) 2021